

PCT

WORLD INTELLECTUAL PROPERTY ORGANIZATION  
International Bureau




INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification <sup>7</sup> : <b>A61B</b>	<b>A2</b>	(11) International Publication Number: <b>WO 00/65981</b> (43) International Publication Date: 9 November 2000 (09.11.00)
(21) International Application Number: PCT/US00/11943 (22) International Filing Date: 1 May 2000 (01.05.00) (30) Priority Data: 60/131,811 30 April 1999 (30.04.99) US (71)(72) Applicants and Inventors: BHADRA, Niloy [US/US]; 3358 DeSota Avenue, Cleveland Heights, OH 44118 (US). KEITH, Michael, W. [US/US]; 65 Meadow Hill Lane, Moreland Hills, OH 44022 (US). KILGORE, Kevin, L. [US/US]; 22960 Summerland, North Olmsted, OH 44070 (US). PECKHAM, P., Hunter [US/US]; 3361 E. Monmouth Road, Cleveland Heights, OH 44118 (US). STAGE, Thomas [US/US]; 1645 Rydalmount, Cleveland Heights, OH 44118 (US). (74) Agents: LONGMUIR, Jeanne, E. et al.; Calfee, Halter & Griswold LLP, 1400 McDonald Investment Center, 800 Superior Avenue, Cleveland, OH 44114 (US).		(81) Designated States: AU, CA, US, European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).  Published <i>Without international search report and to be republished upon receipt of that report.</i>

(54) Title: SURGICAL TOOLS

## Schematic of Prototype IJAT

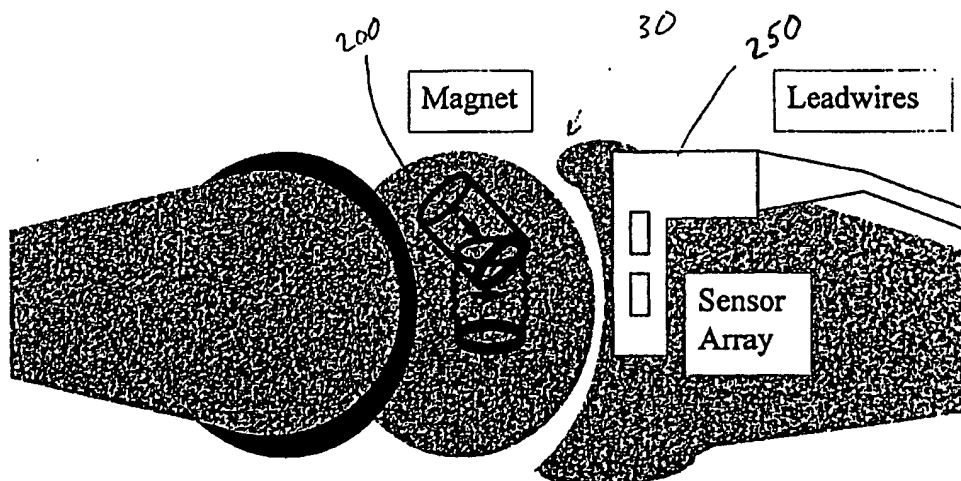

(57) Abstract

A surgical tool set is provided for the preparation of two living bones for the implantation of a medical device including first portion magnet system and a second portion sensor system. The tool set also provides tools for implanting the magnet system and sensor system into living bone. The tool set includes a centering jig and a fork shaped jig, as well as a magnet insertion tool and a sensor insertion tool.

BEST AVAILABLE COPY

*FOR THE PURPOSES OF INFORMATION ONLY*

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece	ML	Mali	TR	Turkey
BG	Bulgaria	HU	Hungary	MN	Mongolia	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MR	Mauritania	UA	Ukraine
BR	Brazil	IL	Israel	MW	Malawi	UG	Uganda
BY	Belarus	IS	Iceland	MX	Mexico	US	United States of America
CA	Canada	IT	Italy	NE	Niger	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NL	Netherlands	VN	Viet Nam
CG	Congo	KE	Kenya	NO	Norway	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NZ	New Zealand	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	PL	Poland		
CM	Cameroon	KR	Republic of Korea	PT	Portugal		
CN	China	KZ	Kazakhstan	RO	Romania		
CU	Cuba	LC	Saint Lucia	RU	Russian Federation		
CZ	Czech Republic	LI	Liechtenstein	SD	Sudan		
DE	Germany	LK	Sri Lanka	SE	Sweden		
DK	Denmark	LR	Liberia	SG	Singapore		
EE	Estonia						

**Title of the Invention****SURGICAL TOOLS****Field of the Invention**

This invention generally relates to surgical tools and more specifically to  
5 tools and a method used for implanting medical devices within bone.

**Background of the Invention**

Injury to the spinal cord of humans and animals has been known to  
cause paralysis. However, muscle movement may still be achieved by direct  
electrical stimulation to the muscle. Stimulation has been provided in humans  
10 and animals using various electrical stimulation devices are known to provide  
such muscle movement. For example, U.S. Patent No. 5,167,222 discloses a  
well known functional neuromuscular stimulation system. Such systems  
typically include a implantable stimulator telemeter devices (IST). The IST is  
powered through a transcutaneous radio-frequency link which also controls the  
15 IST from an external control unit. Wires run from the IST to various muscles of  
the body which are to be stimulated.

However, to optimize the usage of an IST it is important to obtain  
feedback information regarding muscle movement. Thus, a sensor, or sensor  
system, which may detect the relative motion between bones or muscles is used.  
20 A common type of sensor system is a combination of a magnet and a magnetic  
field (Hall Effect) sensor. The Hall Effect sensor can detect motion of the  
magnet and can send an electrical signal to a processor. The electrical signal  
can be used to control the actions of the IST.

Tools exist for placing simple attachments onto bones. For example, a  
25 miniature screwdriver may be used to insert bone screws into bones. The  
situation is more complex however when the elements to be implanted are a  
sensor system including magnets. Electrical leads typically extend from an end  
of the sensor. Thus, common insertion tools which mate with the end of an  
element cannot be used. A cannulated or tubular device must be used.  
30 Cannulated drills and taps have been used in the area of orthopedic  
fracture treatment. However, these tools are not adapted for the process of  
implanting delicate transducer devices of the type disclosed in U.S. Patent No.  
5,167,229.

Improved tools and a method for inserting sensor systems with magnets  
35 using these tools is desired.

### Summary of the Invention

The present application provides improved surgical tools, a surgical tool  
set, and an improved method for use in implantation of a medical device into  
living bone.  
40 The improved tool set allows small and delicate medical devices to be  
implanted into living bone.

Further, use of the improved tool set and method allows devices to be  
implanted into living bone without substantially disturbing the surrounding  
tissue.

45 Further advantages of the present invention will become apparent to  
those of ordinary skill in the art upon reading and understanding the following  
detailed description.

### Brief Description of the Figures

- FIG. 1 is a schematic view of two bones within which an Implantable  
50 Joint Angle Transducer is implanted;
- FIGS. 2 top view of a tool set;
- FIG. 3 is schematic view of a fork shaped jig and drill guide tools shown  
adjacent the bones to be implanted;
- FIGS. 4A and 4B are side and top views, respectively, of a centering jig  
55 tool;
- FIGS. 5A-5C are top, side, and end views, respectively, of a cannulated  
tap;
- FIGS 5D and 5E are top and side views of the portion of the cannulated  
tap cut-away in Figures 5A and 5B respectively.
- 60 FIGS. 6A-6J illustrate various views of components of a magnet  
insertion tool;
- FIGS. 7A-7 are top, side, cut-away side and end views of a sensor  
insertion tool;
- FIG. 8 is a schematic illustration of the magnet system to be implanted  
65 using the tool set of the present application;
- FIG 9 is a schematic illustration of the sensor systems to be implanted  
using the tool set of the present application;
- FIG 10 illustrates the bones to be implanted using the tool set of the  
present application where an incision may be made along the dashed lines I in  
70 the covering tissue to expose the bones;

FIG 11 schematically illustrates a step of the method of the present application using the centering jig tool;

FIG 12 schematically illustrates a step of the method of the present application including drilling and tapping of a first bone to be implanted;

75        FIG 13 schematically illustrates a step of the method of the present application including drilling and tapping of a second bone to be implanted;

FIG. 14 schematically illustrates a step of the method of the present application including insertion of a sensor system into a second bone; and,

80        FIG 15 schematically illustrates a step of the method of the present application including insertion of a magnet system into a first bone using a magnet insertion tool of the present application.

### **Detailed Description of the Preferred and Alternate Embodiments**

Implantable Joint Angle Transducers (IJAT) are used to obtain  
85    information in an electronic form. This information relates to the relative motion between muscles or bones. The IJAT are implanted into living bone as shown in FIG. 1. Described below are innovative tools for implanting IJAT into living bone and a method of implantation using these tools.

#### **Tools**

90        Referring to the drawings, FIGS. 2 and 3 illustrate a preferred tool set 50 according to the invention. The tool set 50, as described in more detail below, includes two or more guide wires 52, a centering jig 70, a screwdriver handle 80, one or more cannulated drills 90, one or more cannulated taps 100, a T-handle 110, a magnet insertion tool 120, a sensor insertion tool 170, and a

95     forked shaped jig 190. The tool set 50 is used to implant a medical device in adjacent living bones. The illustrated bones are the radius R and the lunate L in a human wrist joint. The medical device illustrated includes a first portion which is a magnet system 200 and a second portion illustrated as a sensor system 250 as illustrated. The first portion 200 of the medical device is  
100     implanted in the lunate L bone. The second portion of 250 of the medical device is implanted in the radius R bone.

           Included in the tool set 50 are one or more guide wires 52. The guide wires 52 are attached to the bone in a desired location. The guide wires 52 then are used to guide the cannulated drills 90 and cannulated taps 100 to the desired  
105     location on the bone. The guide wire 52 is preferably thin and has a threaded end. The guide wire 52 is also resilient and will not kink even when bent at extreme angles. Preferably the guide wire 52 is metallic, however it may be made of any material which is easily distinguishable on an X-Ray image.

           Included in the tool set 50 is a centering jig 60 shown in detail in FIG 4.  
110     The centering jig 60 is uniquely designed for the process of implantable joint angle transducer 30 implantation. The centering jig 60 is used as a guide for placing the guide wire 52 into contact with the bone. The centering jig 60 includes an elongate shaft 62, neck 68 and head 74. The elongate shaft 62 has a first end 63 and a second end 64. The first end 63 is machined in order to be  
115     attachable to the screwdriver handle 80 or T-handle 110. The second end 64 is attachable to the neck 68. The elongate shaft 62 and neck 68 are oriented along a common line. The elongate shaft 62 is attached to the neck 68 using a pin, but a screw, force fit, weld or similar means may also be used. The neck 68 has a

diameter, a first end 69 and a second end 70. The second end 70 is attached to  
120 the head 74. The position of the head 74 is angled with respect to the line upon  
which the neck 68 and elongate shaft 62 lie. Preferably the second end 70 is  
threaded and screws into the head, but a force fit, weld or similar means may  
also be used. The head 74 is hollow and has a first end 75, a second end 77 and  
a middle 76. In a preferred embodiment the outer diameter of the head 74 is  
125 equal to the outer diameter of the magnet capsule 202. In an alternate  
embodiment, the outer diameter of the head 74 may be any diameter.  
Preferably the middle 76 of the head 77 is attached to the neck 68. The first end  
75 of the head 74 is equipped with a plurality of teeth 78. The teeth 78 are able  
to adhere to bone. The guide wire 52 may be passed through the hollow head  
130 74. Preferably the centering jig 60 is made of stainless steel, however it may be  
made of any material which is easily distinguishable on a X-Ray image.

The tool set 50 includes one or more cannulated drills 90. The bore size  
of the cannulated drills 90 may vary. The cannulated drills 90 are hollow and  
may consist of varying bore sizes. Each cannulated drill 90 has a first end 91  
135 and second end 92. The first end 91 is attachable to a handle 82 and the second  
end is fluted.

The tool set 50 includes one or more cannulated taps 100 as shown in  
detail in FIG. 5A-5E. The cannulated taps 100 are hollow and may consist of  
varying thread sizes. Each cannulated tap 100 has a first end 101 and second  
140 end 102. The first end is attachable to a handle 82. The second end 102 has four  
longitudinal flutes 103 and is threaded.

The tool set 50 includes a magnet insertion tool 120 as shown in detail in FIGS. 6A-6K. The magnet insertion tool is able to hold the magnet capsule 202 while allowing rotation of the magnet capsule 202 in either a clockwise or counter clockwise direction. The magnet insertion tool 120 is comprised of a collet 130, a center shaft 122, an outer shaft 140, a locking shaft 150, and a rotating handle 160. The magnet insertion tool 120 is able to release the magnet capsule 202 by simply moving the rotating handle 160. The collet 130 as shown in FIGS 6A, 6B, 6J, and 6K has a circular cross section, an exterior surface 133 and a first end 131 and second end 132. The first end 131 is hollow, having an outer sleeve 134, which has an outside surface 135. The outer sleeve 134 is expandable in order to hold and release the magnet capsule 202. The first end 131 is flared and the outer sleeve 134 is comprised of a plurality of tines 136. When expanded, open space appears between the tines 136. When contracted, each tine 136 abuts an adjacent tine 136. One tine 136 includes an aperture 137. An alignment pin 138 may be seated within the aperture 137 and when seated extends into the interior of the outer sleeve 134. The alignment pin 137 may be used to align the magnet capsule 202 when the magnet capsule 202 is held within the outer sleeve 134. The second end 132 of the collet 130 is attachable to the center shaft 122. The collet 130 may be attached to the center shaft 122 using a pin, screw, force fit, weld or similar means. Preferably the collet 130 is made of stainless steel, however it may be made of any material which is easily distinguishable on a X-Ray image.

The center shaft 122 as shown in FIGS 6C-6E is elongated and has a first end 123 and second end 124. The first end 123 is attached to the collet 130

while the second end 124 is attached to the locking shaft 150. Preferably the center shaft 122 is attached to the locking shaft 150 with a set screw.

The outer shaft 140, as shown in FIG 6F, is elongated and has a first end 141 and second end 142. The outer shaft 140 is hollow and may slide along the exterior surface of the center shaft 122. Upon sliding the outer shaft 140 acts as a ferrule, opening and closing the multiple tines 136 of the collet 130. The first end 141 of the outer shaft 140 is chamfered in order to allow smooth contact with the exterior surface of the outer sleeve 134. The first end 141 of the outer shaft 140 may be pushed against the exterior surface of the outer sleeve 134, thus forcing the tines 136 together. The first end 141 of the outer shaft 140 may also be pulled away from the exterior surface of the outer sleeve 134, thus allowing the tines 136 to expand. The second end 142 of the outer shaft 140 is flared outwardly allowing the outer shaft 140 to abut against the rotating handle 160.

The locking shaft 150 as shown in FIG 6H, is elongated and has a first end 151, a second end 153 and a central nub 152. The locking shaft 150 is hollowed from the first end 151 partially through the central nub 152. The center shaft 122 may be inserted into the hollowed area of the locking shaft 150 and attached using a set screw. The first end 151 of the locking shaft 150 is threaded for attachment to the rotating handle 160. The second end 153 is attachable to a handle 82.

The rotating handle 160 as shown in FIG 6G, is a hollow shaft having a first end 161, a second end 162, and an outside surface 163. The outside surface 163 may be knurled. The second end 162 contains an internal thread and is

190 movably attached to the locking shaft 150. The first end 161 abuts the outer shaft 140. Upon rotation of the rotating handle 160 on the internal threads, the rotating handle 160 forces the outer shaft 140 to move towards or away from the collet 130.

The collet 130, center shaft 122, outer shaft 140, locking shaft 150, and  
195 rotating handle 160 are all preferably made from stainless steel.

The tool set 50 also includes a sensor insertion tool 170, as shown in FIGS 7A-7D. The sensor insertion tool 170 is a shaft including a first end 171, second end 173, trough 172, and a keyed portion 174. The second end 174 is attachable to a handle 82. The keyed portion 174 is at the first end 171 of the  
200 sensor insertion tool 170 and the trough 172 is adjacent to the keyed portion 174. The trough 172 is formed of two arched sides 175 and 176 and has a C-shaped cross section and acts as a holder for the leads 256 from the sensor system 250. The keyed section 174 comprises two prongs 177 and 178 which are partial longitudinal extensions of the sides 175 and 176 of the C-shaped  
205 trough 172. The keyed section 174 may be any shape but is preferably T-shaped when viewed perpendicularly to the longitudinal line of the sensor insertion tool 170. The keyed section 174 mates with oval slots 258 upon the sensor system 250 and attaches to the sensor system 250. The top of the T-shaped keyed portion 174 will slide side to side without detachment within the  
210 oval slot 258 depending upon the direction of rotation of the sensor system 250 and sensor insertion tool 170. The sensor system 250 may be detached from the keyed portion 174 when the keyed portion 174 is slid to the center of the oval slot 258 and pulled longitudinally away from the sensor system 250.

The centering jig 60, cannulated drill 90, cannulated tap 100, magnet  
215 insertion tool 120 and sensor insertion tool 170 are all attachable to a handle 82.  
The handle 82, as shown in FIG. 2, can be any type of handle such as a  
screwdriver handle 80 or a T-handle 110. The above mentioned tools are also  
attachable to other implements such as drills, clamps, or robot arms.

The tool set 50 includes a fork jig 190 as shown in FIG. 3. The forked  
220 jig 190 is used in combination with a drill guide 198 to direct a guide wire 52 to  
a bone. The forked shaped jig 190 is a solid having a base 191 and two prongs  
192 and 193. The base 191 has a front surface 194 and a back surface 195 and  
multiple apertures 196 which pass from the front surface 194 to the back surface  
195. The prongs 192, 193 are parallel and extend vertically away from the base  
225 191. One guide wire 52 may pass through one of the apertures 196 then  
allowing placement of a second guide wire 52" within a certain distance from  
the first guide wire 52'. A slot 197 having a width exists between the two  
prongs 192, 193. A tubular drill guide 198 having a width less than or equal to  
the width of the slot 197 is used to direct a guide wire 52 to bone. The tubular  
230 drill guide 197 is placed between the two prongs 192, 193 of the forked shaped  
jig 190.

#### The Device To Be Implanted

The tool set 50 is used to implant a medical device in living bone. The  
device illustrated includes the elements of an implantable joint angle transducer  
235 (IJAT) 30. The IJAT 30 is mounted to adjacent bones and is able to sense  
relative motion. The sensed motion is translated into an electrical signal which  
is sent by leads 256 to the Implantable Stimulator Telemeter or another device

which can process data. The LIAT 30 includes a first portion of the medical device, or a magnet system 200 and a second portion of the medical device or  
240 sensor system 250, as seen in FIG. 8 and FIG. 9, respectively. As described in more detail below, the magnet system 200 includes a permanent magnet 201 (not shown), a magnet capsule 202 and a capsule lid 203. As described in more detail below the sensor system 250 includes one or more sensors 251 (not shown), a sensor capsule 252, a strain relieving sleeve 253 and sensor leads 256.

245 Included in the magnet system is a permanent magnet 201. The permanent magnet 201 may be any shape, but is shown as a cylindrical solid. The permanent magnet 201 is made of Neodymium-Iron-Boron, but may be any magnetic material. The magnet system 200 includes a magnet capsule 202. The permanent magnet 201 is held within the magnet capsule 202. The magnet  
250 capsule 202 is preferably a hollow cylinder having a circular cross section. The magnet capsule 202 has an outside surface 204 which is threaded with a pitch of 32 threads per inch. The leading edge 205 of the magnet capsule is not threaded. One or more longitudinal grooves 206 are cut through the threads on the outside surface 204 for the passage of liquids. The thread size matches the  
255 thread size of the cannulated tap 100. Preferably the magnet capsule 202 is made of titanium. The magnet capsule 202 is simply screwed into place within a bone which has previously been drilled and tapped. The magnet system 200 further includes a magnet capsule lid 203. The magnet capsule lid 203 is preferably a cylindrical solid with a flanged end. The capsule lid 203 further  
260 includes an exterior surface which is slotted and which is placed inside of the

magnet capsule 202 The flanged end of the magnet capsule lid 203 can be easily gripped by the magnet insertion tool 120.

The sensor system 250 is placed adjacent to the magnet system 200 and senses the magnetic field of the permanent magnet 201. The sensor system 250 includes a sensor capsule 252 which is a hollow cylinder with a closed end. Preferably the sensor capsule 252 is made of titanium. The sensor capsule 252 has an outside surface 254 which is partially or completely threaded. Any thread pitch may be used, but a pitch of 14 threads per inch is preferred. One or more longitudinal grooves 255 are cut through the threads on the outside surface for the passage of liquids. The sensor capsule 252 also has two oval slots 258 with longitudinal stems on the outside surface 254. The oval slots 258 mate with the keyed portion 174 of the sensor insertion tool 170. When centered within the oval slot 258, the keyed portion 174 of the sensor insertion tool 170 may be withdrawn through the slot's longitudinal stem. The sensor system 250 also includes one or more sensors 251. Preferably the sensors 251 are one or more Hall Effect sensors in combination with a Hittman hexapolar feedthrough.

Data from the sensors 251 is transmitted to a device electronically through sensor leads 256. The leads 256 are preferably common shielded cables. The sensor system 250 includes a strain relieving sleeve 253 to protect the sensor leads 256. The strain relieving sleeve 253 is a hollow tube which surrounds all leads exiting the sensor capsule 252. The strain relieving sleeve 253 prevents damage to the leads 256 by allowing limited bending of the individual leads 256. The strain relieving sleeve 253 is bendable but resilient.

## METHOD

285 IJAT systems 30 are implanted into bones. For test purposes the IJAT system 30 may be inserted into a non-living bone. IJAT systems 30 are implanted into living human or animal bones. The IJAT system 30 is used in conjunction with an implantable stimulator telemeter, but may be used by itself as well. A method for inserting an IJAT system 30 into living bone is described  
290 below. Also described is a one embodiment of the method where the IJAT 30 is being inserted into the lunate and radius bones of the human wrist.

The process of inserting an IJAT 30 is performed utilizing fluoroscopy so the surgeon performing the insertion may be able to view all tools as well as the IJAT 30. Depending upon the step being performed in the method, the  
295 fluoroscopic views may be in a single plane or bi-planer. In one embodiment, fluoroscopy is performed using a radio-lucent hand table.

The first step, as shown in FIG 10, in the IJAT 30 insertion method is to create an incision in the skin surrounding the bone into which the IJAT 30 will be inserted. In one embodiment of the method the incision is made from the  
300 capito-lunate joint to the radio-carpal joint.

The second step in the IJAT 30 insertion method is to expose the bone into which the IJAT 30 will be inserted. Dissection is kept to a minimum in order keep blood providing arteries functional. In one embodiment, the lunate bone is exposed just proximal to its dorsal pole. In one embodiment the radius  
305 bone is exposed from a point approximately one inch proximal to the wrist joint.

The third step 30, as shown in FIG. 11, in the IJAT insertion method is placement of the centering jig 60 over the first living bone. In one embodiment

of the method, the first living bone is the lunate bone of the wrist. The teeth 78 upon the head 74 of the centering jig 60 are placed in contact with the first  
310 living bone. The centering jig 60 is located in the appropriate position by a surgeon who is able to view the centering jig 60 by fluoroscopy. In one embodiment of the method, the appropriate position is achieved when the lunate bone is visible all around the circle created by the head 74 of the centering jig 60. In one embodiment the head 74 of the centering jig 60 has a length of 0.787  
315 inches and a diameter of 0.177 inches.

The fourth step in the IJAT 30 insertion method is the insertion of the first guide wire 52' into the first living bone. The first guide wire 52' is fed through the hollow head 74 of the centering jig 60. The first guide wire 52', being threaded, may be engaged with the first living bone L. In one  
320 embodiment, the first guide wire 52' is 154 millimeters long and has a diameter of 2 millimeters. A benefit to placing a guide wire 52' is that if the surgeon determines the placement of the guide wire 52 is not appropriate, relocation may be performed without excessive trauma and with minimal damage to the living bone. In one embodiment of the method the first guide wire 52' is placed  
325 into the dorsal surface of the lunate bone.

The fifth step in the IJAT 30 insertion method is the removal of the centering jig 60. The sixth step, as shown in FIG 3, in the IJAT 30 insertion method is the placement of the fork shaped jig 190. The first guide wire 52' is threaded through one of the apertures 196 in the base 191 of the fork shaped jig  
330 190. Placing the first guide wire 52' within the fork shaped jig 190 guarantees that the second guide wire 52'' will be located within a desired distance of the

first guide wire 52'. The seventh step in the IJAT 30 insertion method is the placement of a drill guide 198 within the slot 197 of the fork shaped jig 190. The eighth step in the IJAT 30 insertion method is the placement of the second  
335 guide wire 52. In one embodiment, the second guide wire 52" is 154 millimeters long and has a diameter of 2 millimeters. The second guide wire 52" is threaded through the drill guide 198 and engaged with the second living bone R. In one embodiment of the method the second guide wire 52" lodges in subchondral bone midway between the dorsal and volar cortices.

340 The ninth step as shown in FIG. 12 in the IJAT 30 insertion method is the drilling of the first living bone L. A cannulated drill 90, which circumscribes the first guide wire 52' is used to drill the first living bone L. In one embodiment of the method a 4.5 mm drill is used and the drilling depth does not exceed ten millimeters. In one embodiment, only lateral fluoroscopy is  
345 necessary for viewing the drilling process. The tenth step in the IJAT 30 insertion method is the removal of the cannulated drill 90 and the tapping of the drilled hole. Tapping is performed using a cannulated tap 100 which circumscribes the first guide wire 52". The cannulated tap 100 is driven to the depth to which the hole was drilled. In one embodiment, a 5 millimeter  
350 cannulated tap is used. The eleventh step in the IJAT insertion method is the removal of the first guide wire 52" while leaving the cannulated tap 100 in place.

The twelfth step, as show in FIG 13, in the IJAT 30 insertion method is the drilling of the second living bone R. A second cannulated drill 90' which  
355 circumscribes the second guide wire 52" is used to drill a hole in the second

living bone R. In one embodiment of the method, the hole is drilled in multiple stages to avoid having the drill bit walk. The drilling is performed with a 4.5 millimeter drill, followed by a 6.5 millimeter drill and an 8 millimeter drill is used to overdrill only the cortex portion of the second living bone R. The  
360 thirteenth step in the IJAT 30 insertion method is the removal of the second cannulated drill 90' and the tapping of the drilled hole. Tapping is performed using a second cannulated tap 100' which circumscribes the second guide wire 52". In one embodiment of the method a 6.5 millimeter cannulated tap is used. The second cannulated tap 100' is driven to the depth to which the hole was  
365 drilled.

The thirteenth step in the IJAT 30 insertion method is the removal of the second cannulated tap 100' and the second guide wire 52" and the insertion of the sensor system 250, as shown in FIG. 14. The sensor system 250 is attached to the sensor insertion tool 170. The sensor system 250 is then threaded into the  
370 tapped hole in the second bone R. Once in position the keyed section 174 of the sensor insertion tool 170 is centered within the oval slot 258 upon the sensor capsule 252 and the sensor insertion tool 170 is detached. The fourteenth step in the IJAT 30 insertion method is to electrically connect the sensor leads 256 to the implantable stimulator telemeter or other device.

375 The fifteenth step in the IJAT 30 insertion method is the removal of the cannulated tap 100 from the hole in the first living bone L and the insertion of the magnet system 200, as shown in FIG. 15. The magnet system 200 is implanted using the magnet insertion tool 120. The magnet system 200 is placed into a desired position as determined by feedback from the sensor 251

380 and the implantable stimulator telemeter or other device. The axis of the permanent magnet 201, which runs perpendicular to a long axis of the magnet capsule 202, is oriented with either north or south facing the sensor 251 to get the signals from the sensor 251 as close to the center of a 12 bit AD range as possible.

385 Although the device and method have been shown and described with reference to certain embodiments minor variation and insubstantial differences in the various combination of materials and methods of application may occur to those of ordinary skill in the art while remaining within the scope of the invention as claimed and equivalents.

### Claims

1. A surgical tool set used to prepare said first bone for accepting a first portion of a medical device and a second bone for accepting a second portion of a medical device, and for inserting said first portion of a medical device into a first bone and a second portion of a medical device into said second bone, said surgical tool set comprising:

a centering jig having an elongate shaft, a neck and a hollow head;

a first magnet insertion tool having a collet, a center shaft, an outer shaft, a locking shaft, and a rotating handle;

a second insertion tool having a shaft with a first end, a second end, a trough section, and a keyed section; and

a fork jig having a base portion and first and second prongs extending therefrom.

2. The tool set of claim 1 wherein said centering jig further provides a handle mounted on said elongated shaft;

said centering jig neck having a first and second end, said first end for engagement with said elongate shaft and said second end for engagement with said hollow head,

said hollow head having a first end and a second end, said hollow head for engagement with said neck, and said hollow head first end having a plurality of teeth for securing engagement with said first bone.

3. The tool set of claim 1 wherein said first insertion tool further provides a circular cross section on said collet having first and second ends, said first end of said collet being flared and consisting of a plurality of tines, one of said tines having a hole for receiving an alignment pin and said second end of said collet for engagement with said center shaft, said center shaft of said first insertion tool having a first end and a second end, said first end of said center shaft for

engagement with said collet and said second end of said center shaft for engagement with said locking shaft;

said outer shaft of said first insertion tool being hollow and having a first end and a second end, said second end of said outer shaft abutting said rotating handle, said first end of said outer shaft being chamfered and said second end of said outer shaft being flared outwardly,

said locking shaft of said first insertion tool having a first end and a second end, said first end of said locking shaft being threaded for engagement with said rotating handle and said second end of said locking shaft for engagement with a handle, said locking shaft being hollow through said first end of said locking shaft to receive said center shaft, and said rotating handle having a first end and a second end where said first end of said rotating handle abuts said outer shaft and said second end of said rotating handle includes a threaded portion for threaded engagement with said locking shaft.

4. The tools set of claim 1 further including a cannulated tap tool having a first end and a second end, said first end having four flutes and a threaded portion and said second end adapted for engagement with a handle;

5 The tool set of claim 1 wherein said centering jig further provides said hollow head with an outer diameter and a first portion of a medical device having an outer diameter equal to said outer diameter of said hollow head.

6. The tool set of claim 1 wherein said trough section of said second insertion tool is C-shaped and includes two arch side portions, and said keyed section comprises two T-shaped extensions extending longitudinally from said arch side portions of said trough section, and said second end of said second insertion tool is adapted for engagement with a handle.

7. The tool set of claim 1 wherein said fork jig base includes a front surface, a back surface, having a front surface and a back surface; multiple apertures through said front surface to said back surface, and a slot intermediate said first and second prongs.
8. The tool set of claim 7 further including a drill guide tool which includes a tube having an outside diameter, and said outside diameter is less than or equal to the width of said slot between said first and second prongs.
9. A method for inserting a magnet system into a first living bone and a sensor system into a second living bone comprising:
- a) making an incision into tissue in an area covering said first and second living bones;
  - b) exposing said first and second living bones;
  - c) placing a centering jig tool over a surface of said first living bone;
  - d) inserting a first guide wire into said centering jig and extending said first guide wire into engagement with said first living bone;
  - e) removing said centering jig and leaving said first guide wire engaged with said first living bone;
  - f) placing a fork jig having multiple apertures and a slot adjacent to said second living bone such that said first guide wire passes through one of said multiple apertures;
  - g) placing a drill guide within said slot of said fork jig;
  - h) placing a second guide wire within said drill guide and extending said second guide wire into engagement with said second living bone;
  - i) guiding a first cannulated drill, circumscribing said first guide wire, into engagement with said first living bone and drilling a hole into said first living bone;

j) removing said first cannulated drill and guiding a first cannulated tap, into engagement with said first living bone and tapping said first living bone;

k) removing said first guide wire;

l) guiding a second cannulated drill, circumventing said second guide wire, into contact with said second living bone and drilling a hole into said second living bone;

m) removing said second cannulated drill and guiding a second cannulated tap, circumventing said second guide wire, into engagement with said second living bone and tapping said second living bone;

n) removing said second cannulated tap from said second living bone;

o) inserting said sensor system into said first living bone using a sensor insertion tool;

p) connecting electrically said sensor system to an implantable stimulation device;

q) removing said first cannulated tap from said first living bone and inserting said magnet system, using a magnet insertion tool, into a desired position as determined by feedback from said sensor system.

10. The method of claim 9 further comprising the step of utilizing visualizing tools.

11. The method of claim 9 wherein said first living bone is the lunate bone of the human wrist and said second living bone is the radius bone of the human wrist.

12. A centering jig used to prepare a first bone for accepting a magnet system comprising:  
an elongate shaft being mountable to a handle,  
a hollow head having a first end and a second end, said first end having a plurality of teeth for contacting said first bone, and  
a neck having a first end and a second end, said first end being attachable to said elongate shaft and said second end being oppositely attachable to said hollow head.

13. A magnet insertion tool used to insert a magnet system into a first bone comprising:

a collet having a circular cross section and a first end and a second end, said first end of said collet being flared and consisting of a plurality of tines, one of said tines having a hole for receiving an alignment pin and said second end of said collet being attachable to a center shaft;

said center shaft having a first end and a second end, said first end of said center shaft attachable to said collet and said second end of said center shaft attachable to a locking shaft;

an hollow outer shaft having a first end and a second end, said second end of said outer shaft abutting a rotating handle, said first end of said outer shaft being chamfered and said second end of said outer shaft being flared outwardly;

said locking shaft having a first end and a second end, said first end of said locking shaft being threaded for attachment to said rotating handle; and

said rotating handle having a first end and a second end, said first end of said rotating handle abutting said outer shaft and said second end of said rotating handle threaded and attachable to said locking shaft.

14. A sensor insertion tool for inserting a sensor system into a second bone, said sensor insertion tool comprising:


a shaft having a first end, a second end, a troughed section, and a keyed section;

said troughed section is C-shaped and has two arched sides;

said keyed section comprises two T-shaped extensions extending longitudinally from said arched sides of said troughed section; and

said second end is attachable to a handle.

# Schematic of Prototype IJAT

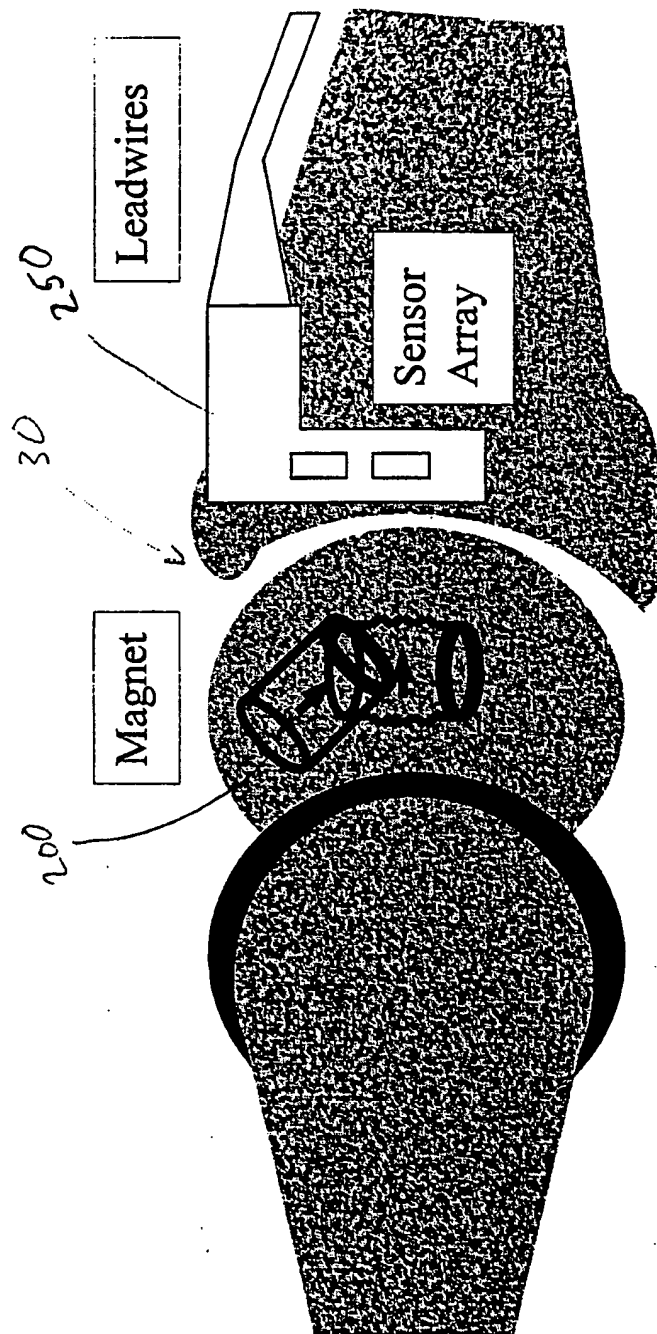

F161



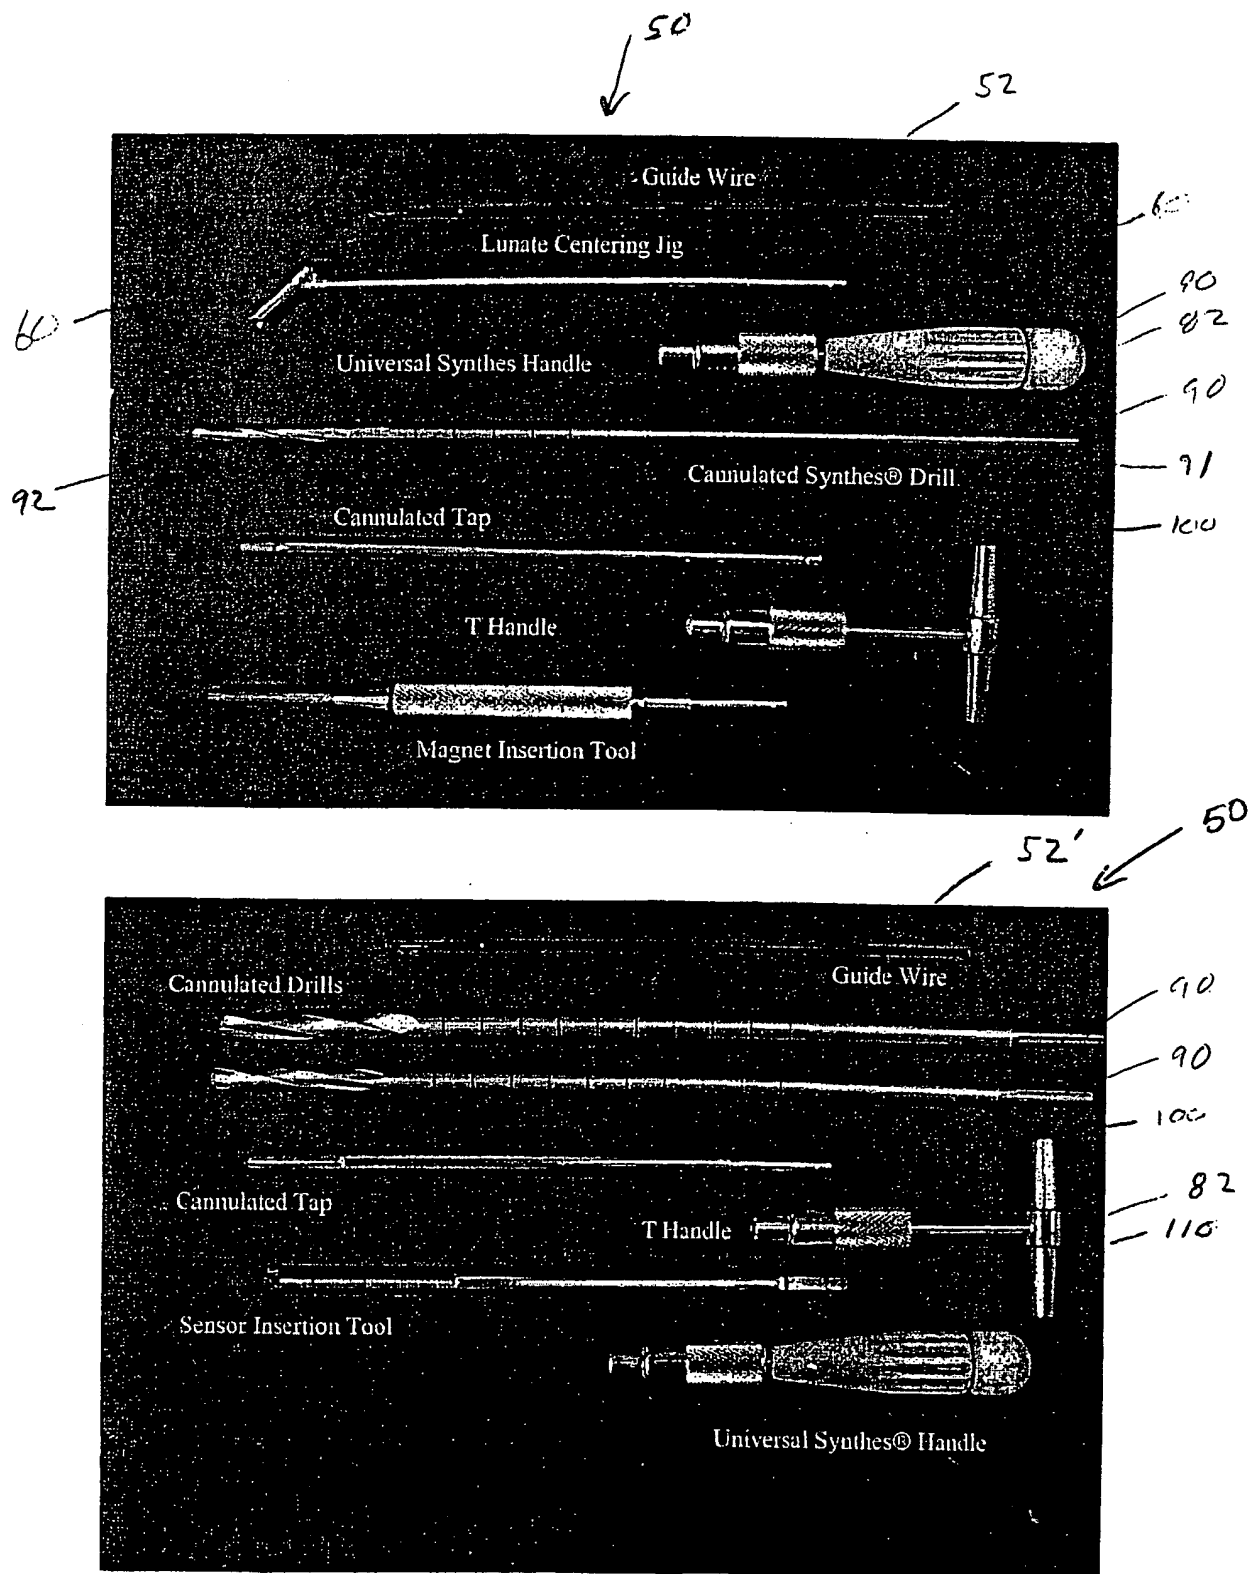


FIG. 2

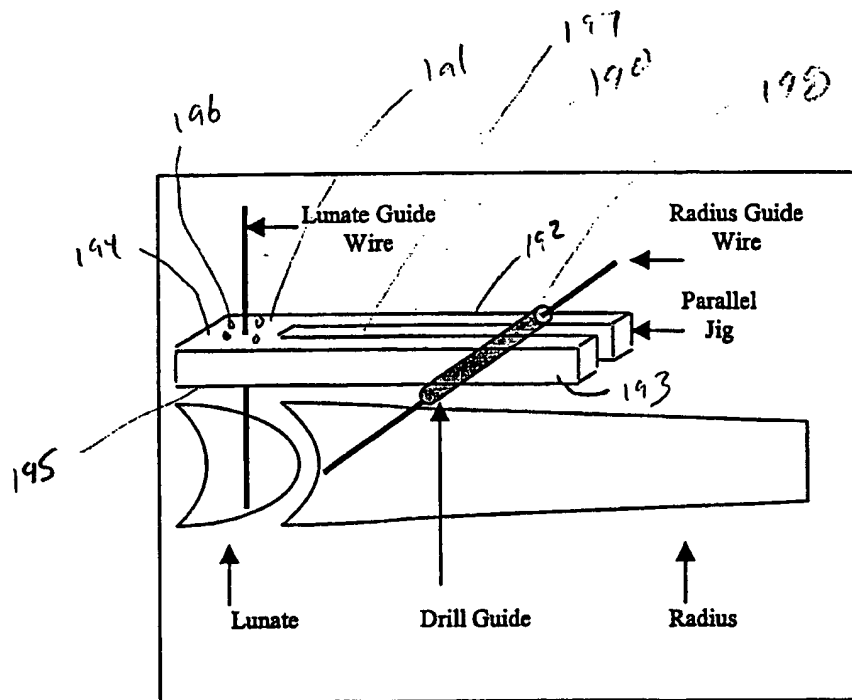

F16.3

# Guide Wire X-ray Alignment Jig

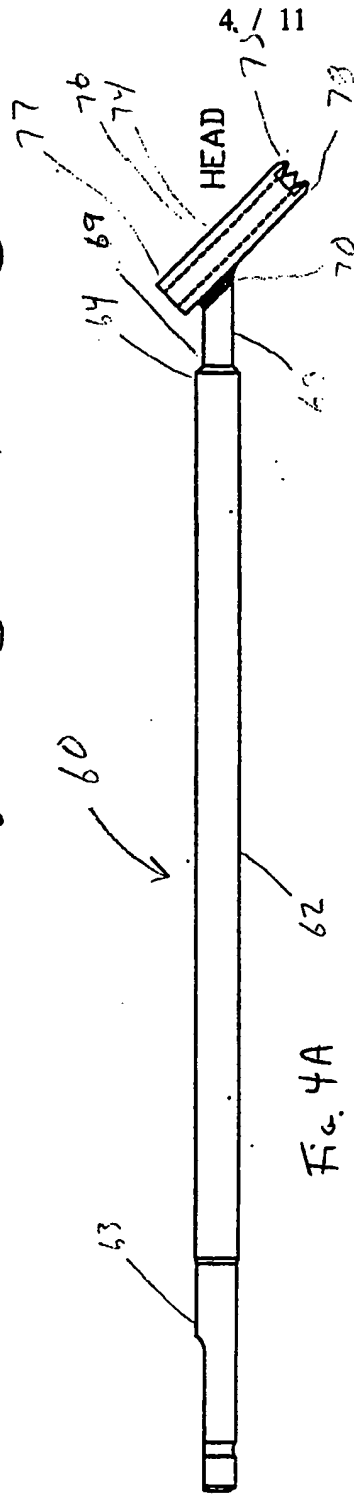

LOCKING SHAFT

SHAFT  
2x SIZE

NECK

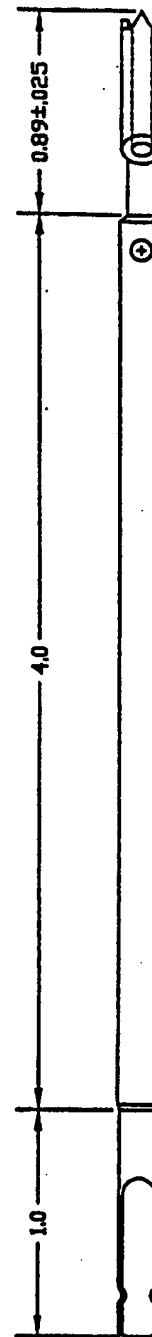


Fig. 4B







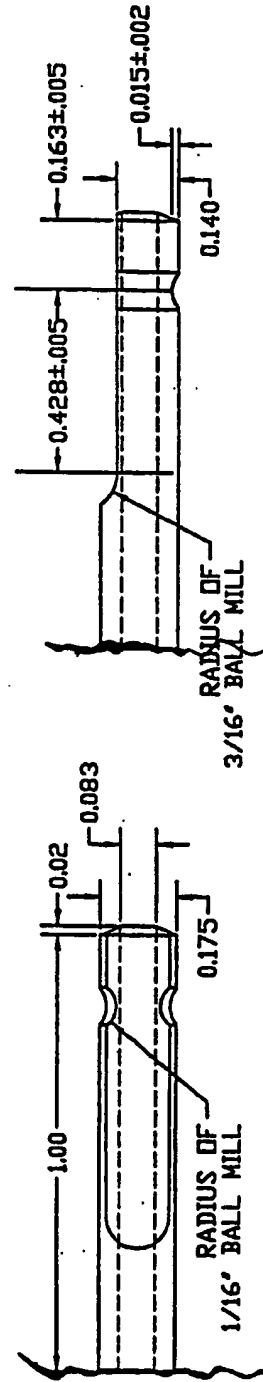


FIG. 5E

FIG. 5D

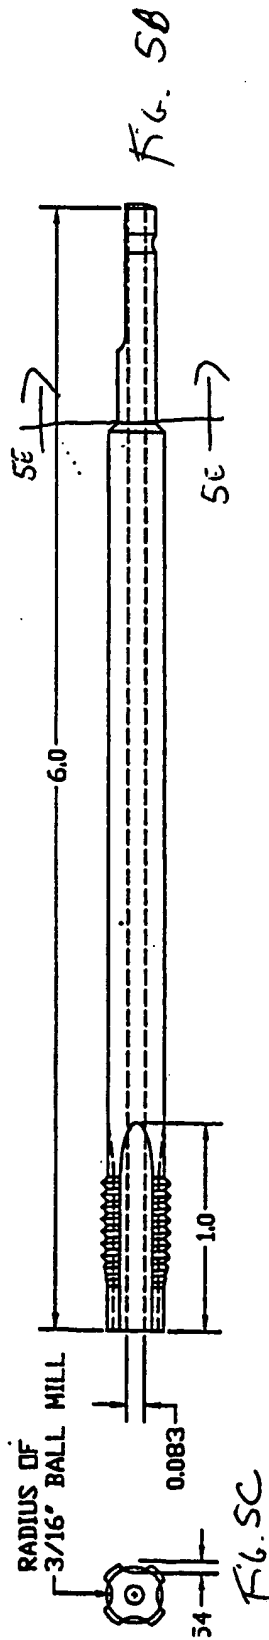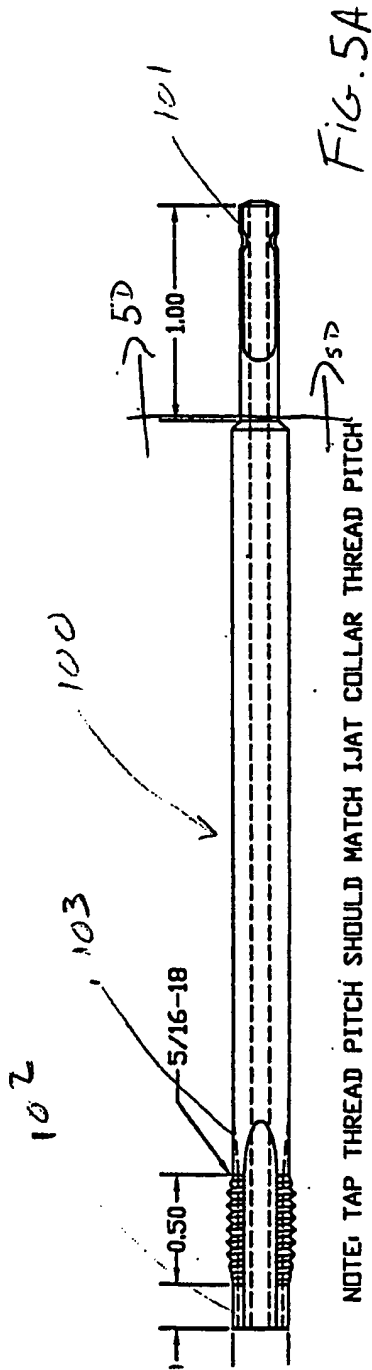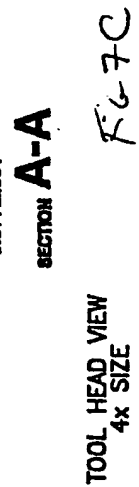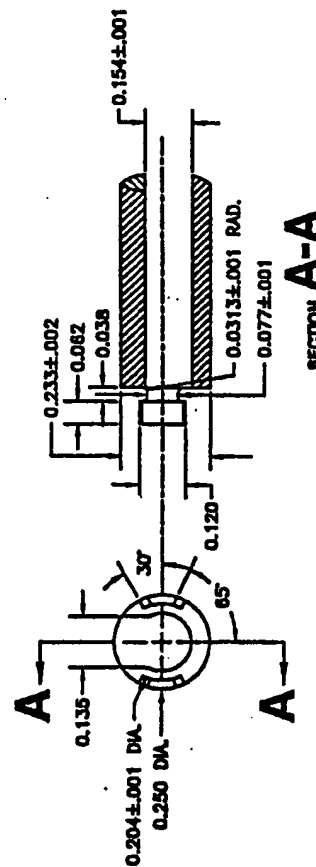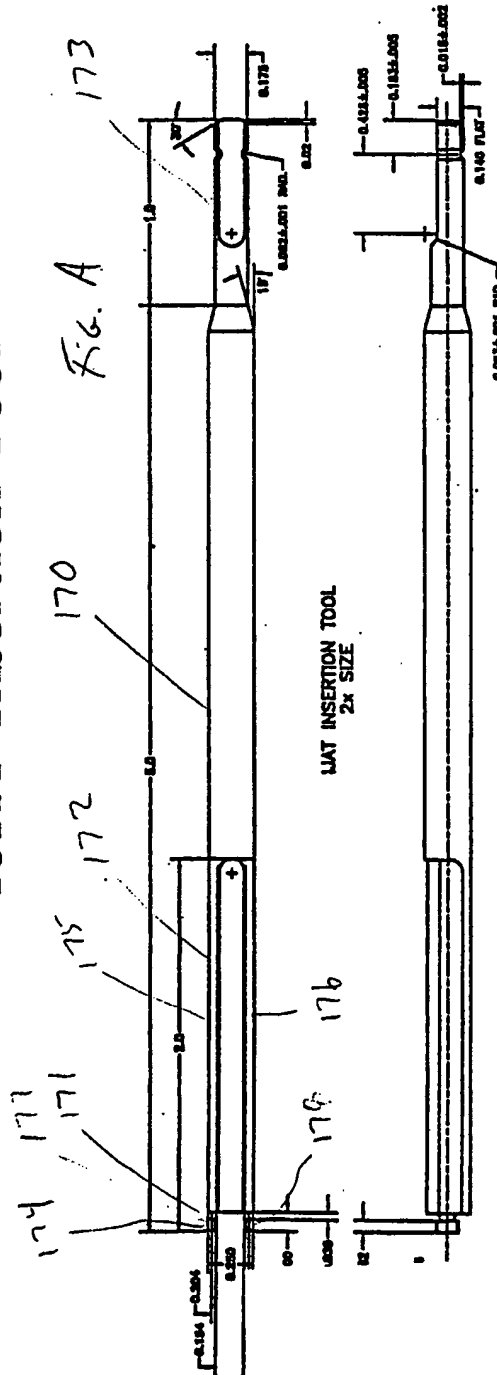

# IJAT Insertion Tool



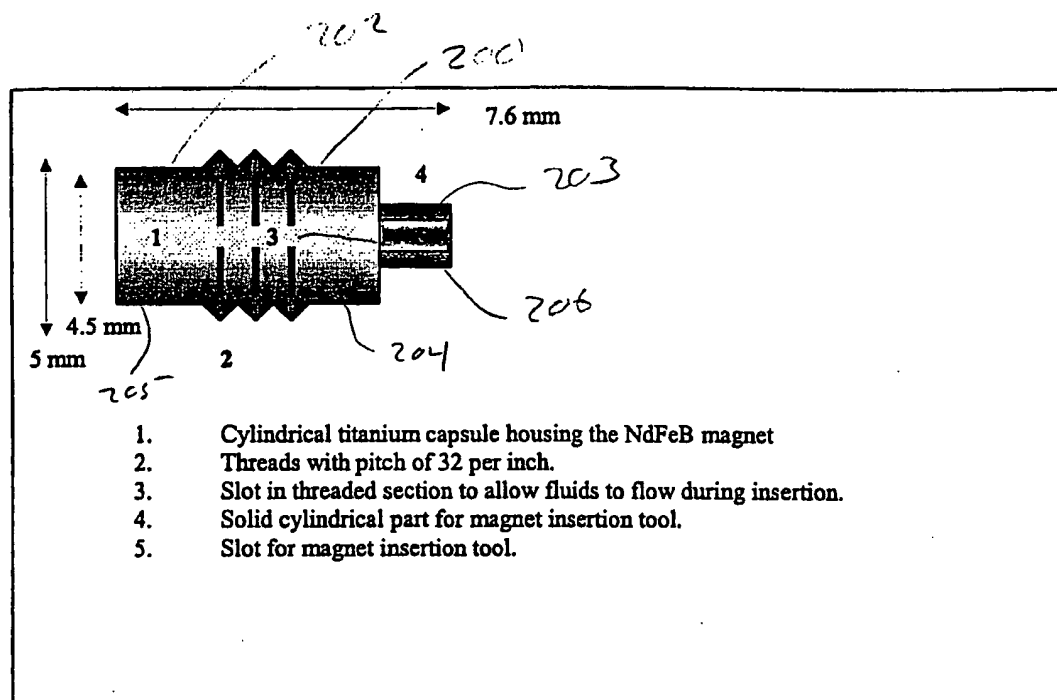


FIG. 8

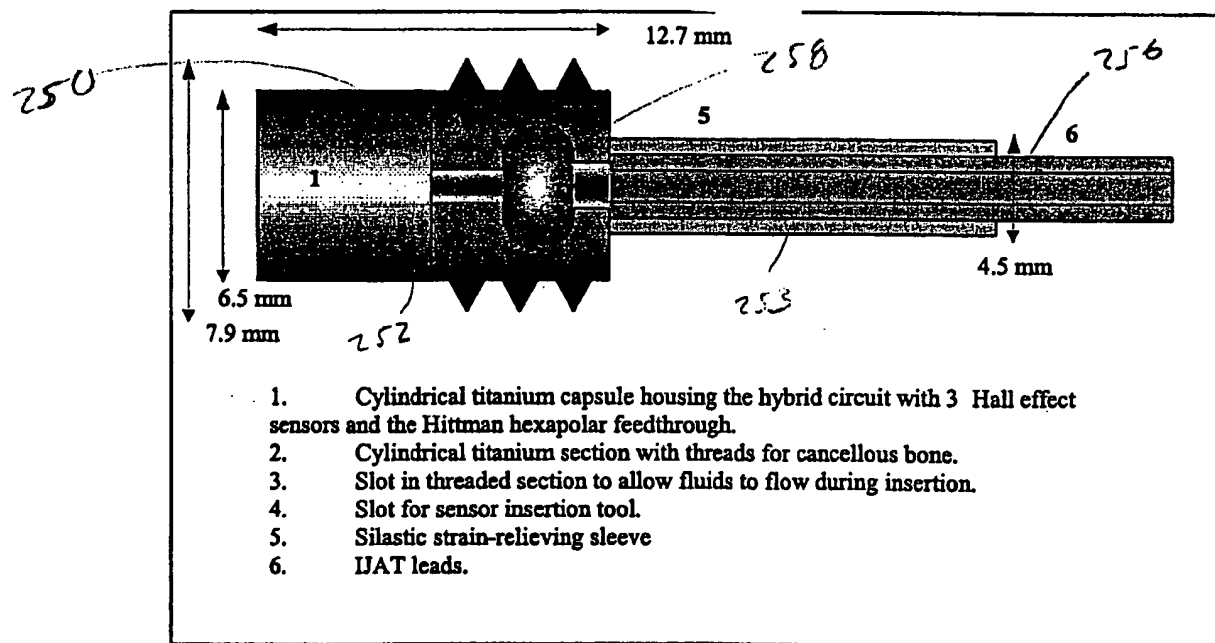


FIG. 9

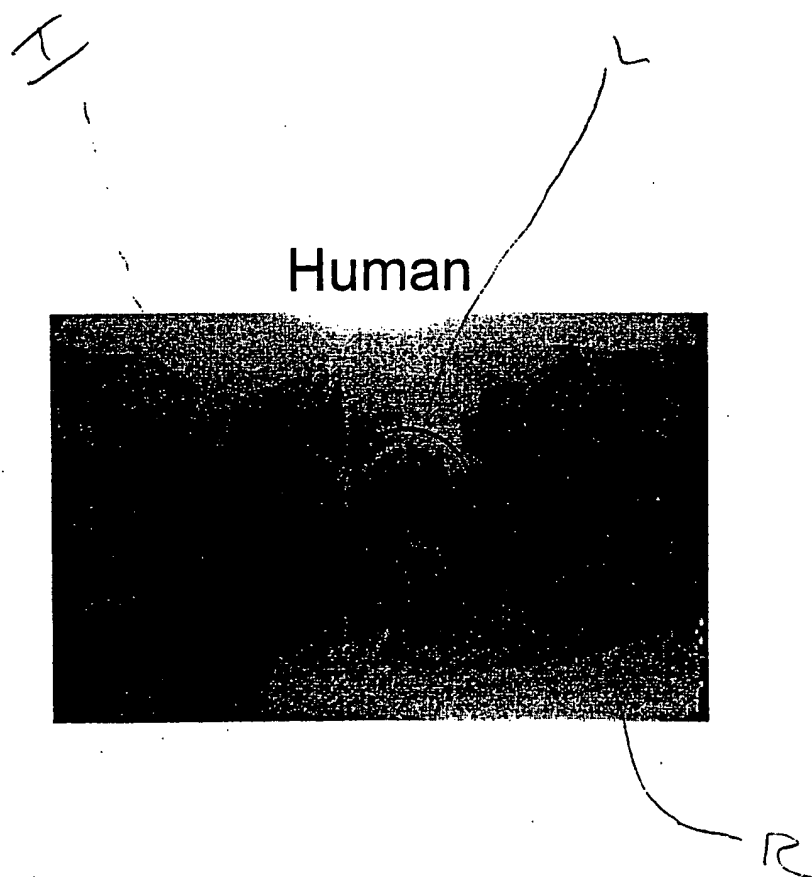


FIG. 10